



**FIG. 1**

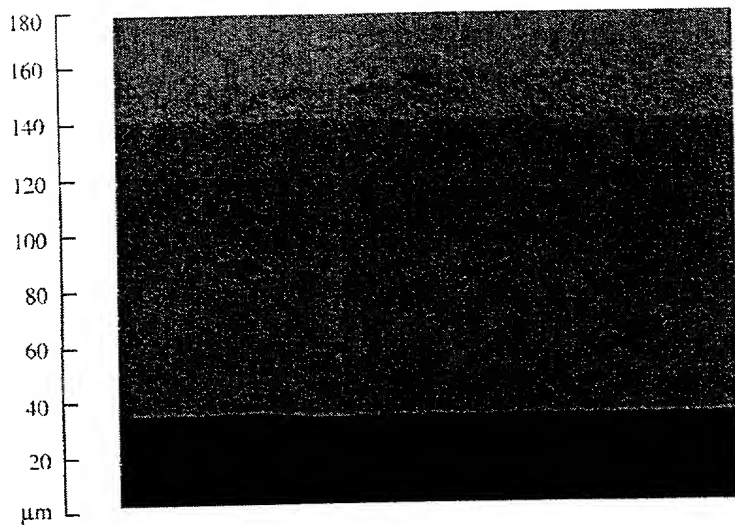

**FIG. 2A**

Sample: TEST


500 X

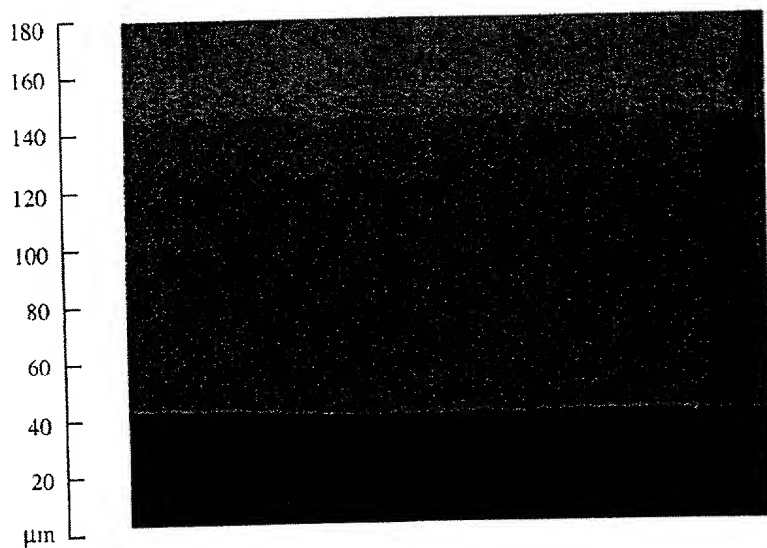

**FIG. 2B**

Sample: CONTROL


500 X

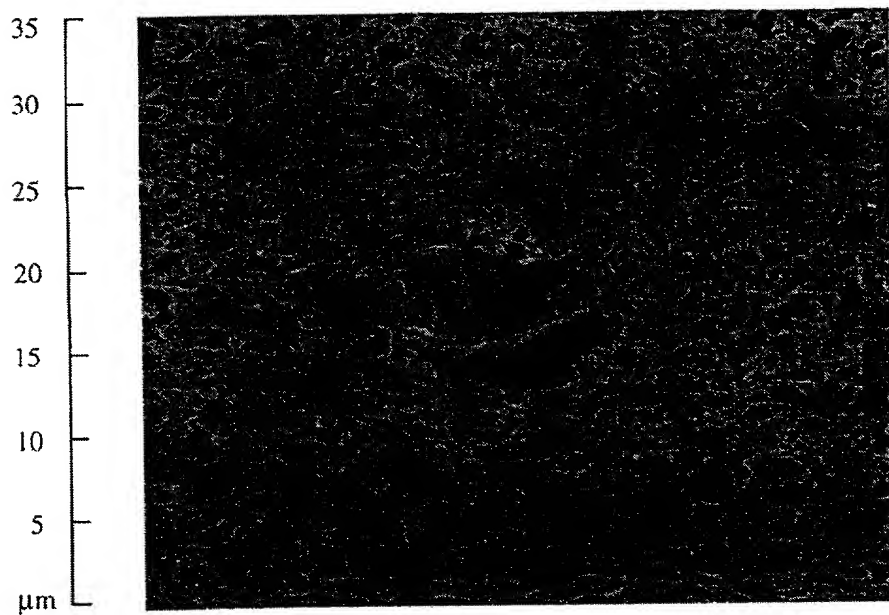

**FIG. 3A**

Sample: TEST


2,500 X

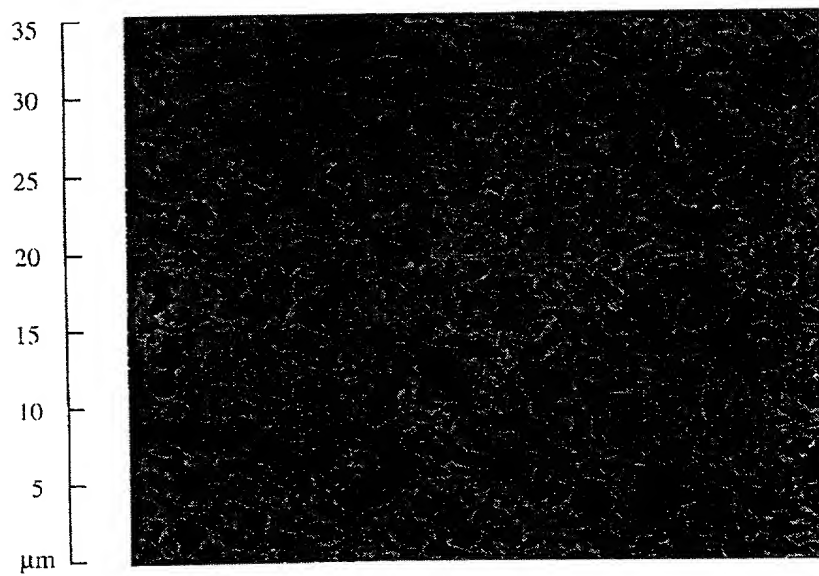

**FIG. 3B**

Sample: CONTROL


2,500 X

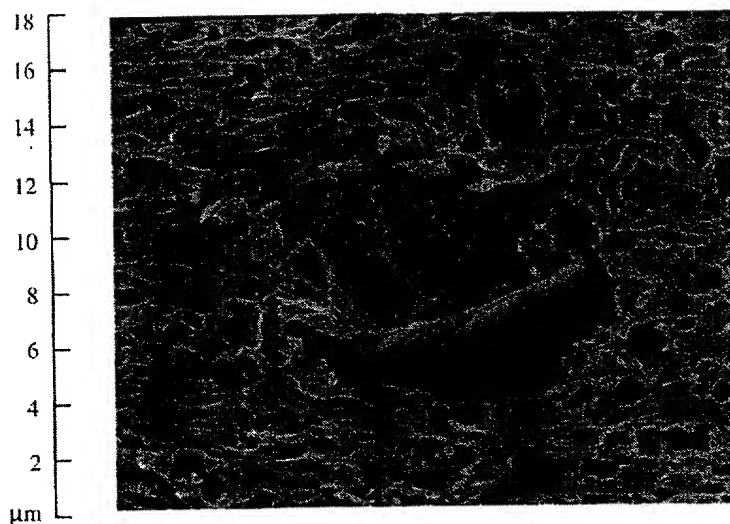

**FIG. 4A**

Sample: TEST

5,000 X

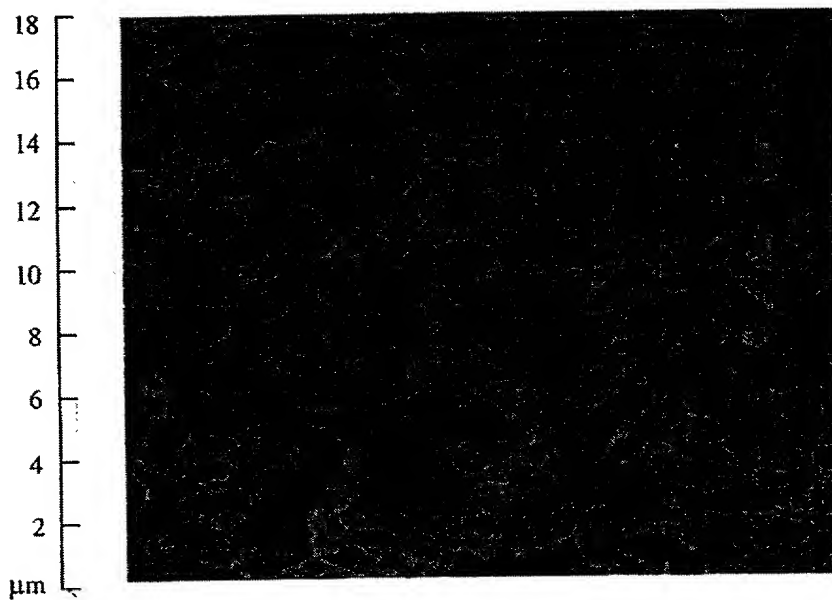

**FIG. 4B**

Sample: CONTROL

5,000 X

M      PCR controls      K562 DNA w/standard  
   membrane      No template  
   controls

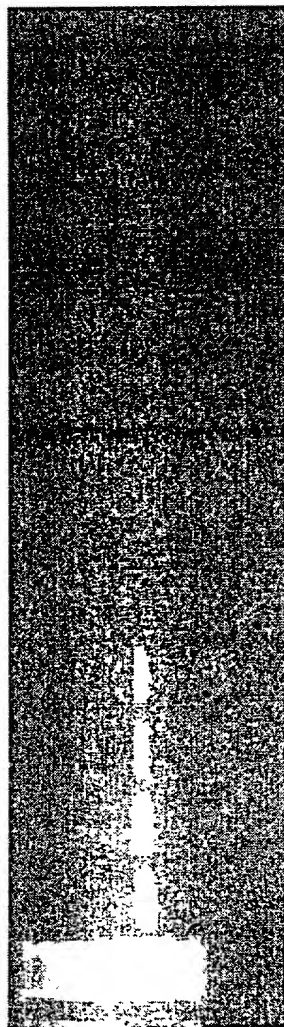


Figure 5

K562 DNA w/ Xtra Bind  
M      nylon membrane



Figure 6